



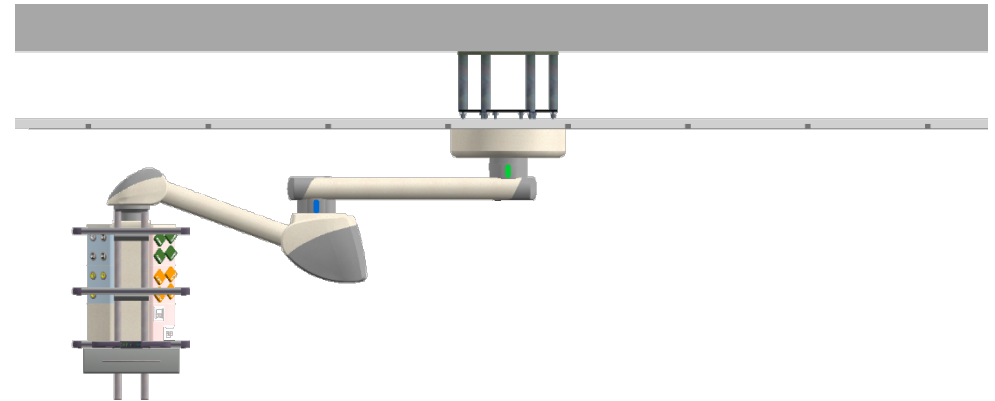

# Configuration proposal General Surgery (CH4)

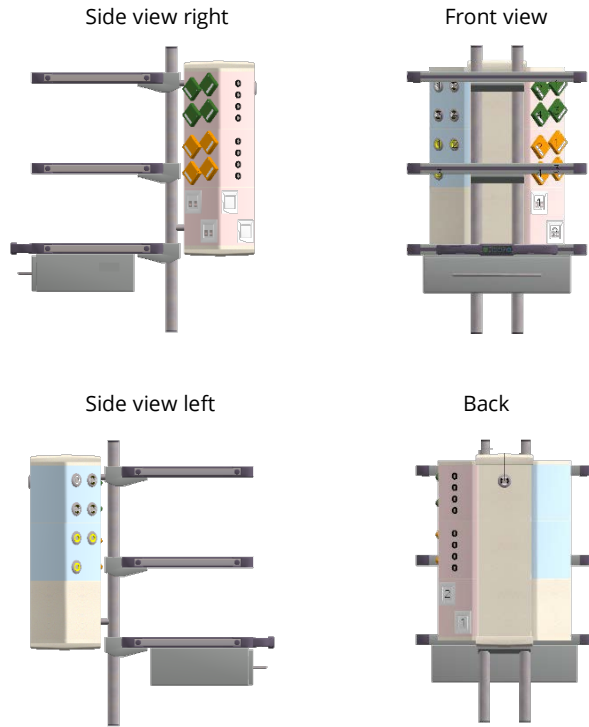

Configuration description:  
 MediLift 1000/1000 with Service Head 600  
 3 x Shelf 520 mm, 1 x Drawer

1. Brake system: Electromagnetic
2. Action space\*: >4,800 mm
3. Weights and Pay Loads  
 Remaining Net Pay Load: 89 kg  
 Max. pendant pay load: 150 kg  
 Vertical force as configured: 3166 N
4. Remaining Diameter: 52 %


Number of service components											
O <sub>2</sub>	Air 4/5	N <sub>2</sub> O	Vac	CO <sub>2</sub>	N <sub>2</sub>	AGSS	Air 8/ Air- motor	Electrical sockets	Earth bonding sockets	Double RJ45	Data prep.
1	3		3				1	8	8	2	2
Greggersen Forano DIN Standard								PEHA			

\* reference: centre of main bearing to centre of shelf




# Configuration proposal General Surgery (CH4)

Side view right

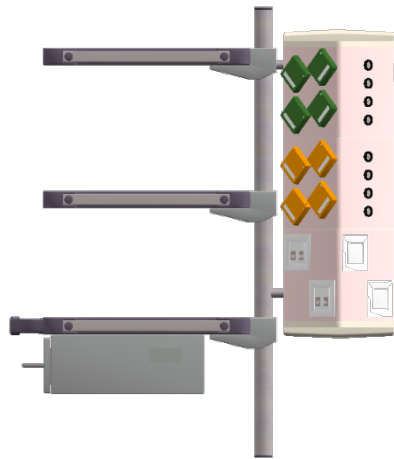


Front view

- |        |   |               |
|--------|---|---------------|
| O2 1   |   | 1 Green       |
| AIR5 2 |   | 2 Green       |
| AIR5 3 |   | 3 Green       |
| AIR5 4 |   | 4 Green       |
| VAC 1  | 1 | 1 Orange      |
| VAC 2  | 2 | 2 Orange      |
| VAC 3  | 3 | 3 Orange      |
|        | 4 | 4 Orange      |
|        |   | 1 2x Cat6 IDC |
|        |   | 2 2x Cat6 IDC |

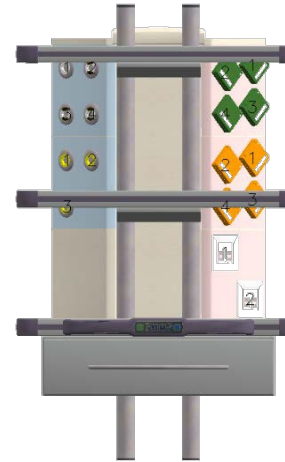

Side view left

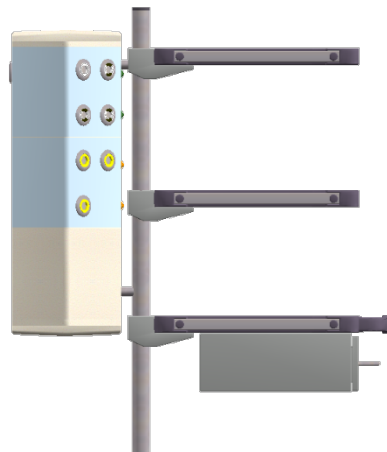

Back

